

Select Calibration Incorporated

213 Fourth St. PO Box 96
 Rodney, Ontario
 NOL 2C0
 (519) 902 7215
 www.selectcalibration.ca

Customer: **Some Company**
 Address: **1024 Binary Way**
Somewhere, Ontario
NOL 2C0
 Contact: **Manager**
 Phone: **519 929 9922 x256**

Machine Model: **Omega**
 Machine Model Id: **24.06**
 Serial Number: **90210**
 Customer Gauge:
 Temperature Min: **20.4 °C**
 Temperature Max: **21.4 °C**

Strict Acceptance:
 1 Point: **0.0046+0.0020L/1000**
 2 Point: **0.0047+0.0019L/1000**

Position Name	Nominal	Measured Length 1	Measured Length 2	Measured Length 3	Uc(k=2)	Tolerance	ABS Dev 1	ABS Dev 2	ABS Dev 3	ABS Dev 1 + Uc(k=2)	ABS Dev 2 + Uc(k=2)	ABS Dev 3 + Uc(k=2)	1 Pt. Strict Acceptance	2 Pt. Strict Acceptance
Position 1	630.0007	629.9969	629.9992	629.9989	0.0014	0.0071	0.0037	0.0015	0.0017	0.0051	0.0029	0.0031	0.0058	0.0059
	1270.0000	1269.9984	1269.9996	1269.9999	0.0024	0.0103	0.0016	0.0004	0.0001	0.0040	0.0028	0.0025	0.0071	0.0071
	1910.0001	1909.9984	1909.9984	1910.0001	0.0036	0.0135	0.0017	0.0017	0.0001	0.0053	0.0053	0.0036	0.0084	0.0084
	2549.9982	2549.9990	2549.9993	2549.9985	0.0047	0.0167	0.0007	0.0010	0.0003	0.0054	0.0057	0.0049	0.0097	0.0096
Position 2	3190.0018	3189.9990	3190.0007	3189.9981	0.0058	0.0199	0.0028	0.0011	0.0037	0.0087	0.0070	0.0096	0.0109	0.0108
	609.9999	610.0022	610.0006	610.0012	0.0014	0.0071	0.0023	0.0007	0.0013	0.0037	0.0020	0.0027	0.0058	0.0059
	1230.0001	1230.0027	1230.0009	1229.9996	0.0024	0.0102	0.0025	0.0008	0.0005	0.0049	0.0032	0.0029	0.0070	0.0070
	1850.0001	1850.0030	1850.0011	1850.0022	0.0035	0.0133	0.0028	0.0010	0.0020	0.0063	0.0045	0.0055	0.0083	0.0082
Position 3	2470.0034	2470.0011	2470.0021	2470.0020	0.0046	0.0164	0.0023	0.0013	0.0014	0.0069	0.0059	0.0060	0.0095	0.0094
	3090.0012	3090.0001	3090.0016	3090.0016	0.0057	0.0195	0.0011	0.0004	0.0004	0.0068	0.0061	0.0062	0.0107	0.0106
	609.9986	610.0006	610.0001	609.9997	0.0014	0.0071	0.0020	0.0015	0.0011	0.0034	0.0029	0.0024	0.0058	0.0059
	1229.9987	1230.0012	1230.0001	1229.9975	0.0024	0.0101	0.0026	0.0015	0.0011	0.0050	0.0039	0.0035	0.0070	0.0070
Position 4	1849.9977	1850.0006	1849.9989	1849.9992	0.0035	0.0132	0.0029	0.0012	0.0015	0.0064	0.0048	0.0050	0.0083	0.0082
	2470.0002	2470.0003	2469.9992	2469.9997	0.0046	0.0163	0.0001	0.0010	0.0005	0.0047	0.0056	0.0051	0.0095	0.0094
	3090.0040	3090.0028	3089.9998	3089.9998	0.0058	0.0195	0.0012	0.0043	0.0043	0.0070	0.0100	0.0101	0.0107	0.0106
	629.9976	629.9999	629.9991	629.9984	0.0014	0.0071	0.0023	0.0015	0.0008	0.0037	0.0029	0.0022	0.0058	0.0059
Position 5[X]	1269.9979	1269.9989	1269.9982	1269.9984	0.0025	0.0103	0.0010	0.0003	0.0006	0.0034	0.0027	0.0030	0.0071	0.0071
	1909.9966	1909.9986	1909.9989	1909.9975	0.0036	0.0135	0.0020	0.0023	0.0009	0.0056	0.0059	0.0045	0.0084	0.0084
	2550.0003	2549.9989	2550.0000	2550.0006	0.0048	0.0167	0.0014	0.0003	0.0003	0.0061	0.0050	0.0051	0.0097	0.0096
	3190.0037	3189.9999	3189.9988	3189.9989	0.0059	0.0199	0.0038	0.0049	0.0048	0.0097	0.0108	0.0107	0.0109	0.0108
Position 6[Y]	299.9999	299.9999	300.0004	300.0003	0.0009	0.0055	0.0001	0.0005	0.0004	0.0010	0.0015	0.0014	0.0052	0.0053
	600.0009	599.9999	600.0004	600.0002	0.0013	0.0070	0.0010	0.0005	0.0006	0.0023	0.0018	0.0020	0.0058	0.0058
	890.0007	889.9996	889.9995	889.9999	0.0018	0.0084	0.0011	0.0013	0.0008	0.0029	0.0030	0.0026	0.0063	0.0064
	1199.9990	1199.9998	1200.0000	1200.0003	0.0023	0.0100	0.0008	0.0010	0.0013	0.0031	0.0033	0.0036	0.0070	0.0070
Position 7[Z]	1499.9966	1500.0005	1500.0014	1500.0008	0.0028	0.0115	0.0039	0.0047	0.0042	0.0067	0.0076	0.0070	0.0076	0.0076
	600.0004	600.0006	599.9999	600.0009	0.0013	0.0070	0.0002	0.0005	0.0005	0.0015	0.0019	0.0019	0.0058	0.0058
	1199.9972	1199.9983	1199.9966	1199.9965	0.0023	0.0100	0.0012	0.0006	0.0007	0.0035	0.0029	0.0031	0.0070	0.0070
	1789.9999	1789.9995	1790.0006	1790.0002	0.0034	0.0130	0.0004	0.0007	0.0003	0.0038	0.0041	0.0037	0.0081	0.0081
Position D1	2399.9983	2399.9994	2399.9985	2400.0007	0.0045	0.0160	0.0011	0.0001	0.0024	0.0055	0.0046	0.0069	0.0094	0.0093
	2999.9998	2999.9986	3000.0019	3000.0007	0.0056	0.0190	0.0012	0.0021	0.0009	0.0067	0.0077	0.0064	0.0106	0.0104
	179.9999	180.0010	180.0014	180.0009	0.0008	0.0049	0.0012	0.0016	0.0010	0.0020	0.0024	0.0019	0.0049	0.0050
	360.0003	360.0007	360.0014	360.0014	0.0010	0.0058	0.0004	0.0010	0.0011	0.0014	0.0020	0.0021	0.0053	0.0054
Position D2	530.0001	530.0003	530.0016	530.0009	0.0012	0.0067	0.0003	0.0016	0.0008	0.0015	0.0028	0.0021	0.0056	0.0057
	719.9999	720.0020	720.0023	720.0015	0.0015	0.0076	0.0020	0.0024	0.0016	0.0035	0.0039	0.0031	0.0060	0.0061
	899.9990	900.0003	900.0009	900.0015	0.0018	0.0085	0.0013	0.0019	0.0024	0.0031	0.0037	0.0042	0.0064	0.0064
	209.9934	209.9929	209.9938	209.9943	0.0020	0.0050	0.0005	0.0004	0.0009	0.0025	0.0024	0.0029	0.0050	0.0051
Position D1	409.9964	409.9984	409.9980	409.9977	0.0022	0.0060	0.0020	0.0016	0.0013	0.0042	0.0038	0.0036	0.0054	0.0055
	610.0008	610.0012	610.0016	610.0016	0.0025	0.0071	0.0004	0.0008	0.0008	0.0029	0.0033	0.0033	0.0058	0.0059
	810.0027	810.0023	810.0019	810.0021	0.0028	0.0081	0.0005	0.0008	0.0006	0.0033	0.0036	0.0034	0.0062	0.0062
	1010.0028	1010.0016	1010.0015	1010.0016	0.0032	0.0091	0.0012	0.0013	0.0012	0.0044	0.0045	0.0044	0.0066	0.0066
Position D2	209.9934	209.9937	209.9931	209.9937	0.0020	0.0050	0.0003	0.0003	0.0003	0.0023	0.0023	0.0023	0.0050	0.0051
	409.9964	409.9973	409.9965	409.9960	0.0022	0.0060	0.0009	0.0000	0.0004	0.0032	0.0023	0.0026	0.0054	0.0055
	610.0008	610.0019	610.0015	610.0009	0.0025	0.0071	0.0011	0.0007	0.0001	0.0036	0.0032	0.0026	0.0058	0.0059
	810.0027	810.0034	810.0029	810.0035	0.0028	0.0081	0.0007	0.0002	0.0008	0.0035	0.0030	0.0036	0.0062	0.0062
	1010.0028	1010.0027	1010.0023	1010.0027	0.0032	0.0091	0.0001	0.0005	0.0001	0.0033	0.0037	0.0033	0.0066	0.0066

Select Calibration Incorporated


213 Fourth St. PO Box 96
 Rodney, Ontario
 NOL 2C0
 (519) 902 7215
 www.selectcalibration.ca

Customer: **Some Company**
 Address: **1024 Binary Way**
Somewhere, Ontario
NOL 2C0
 Contact: **Manager**
 Phone: **519 929 9922 x256**

Machine Model: **Omega**
 Machine Model Id: **24.06**
 Serial Number: **90210**
 Customer Gauge:
 Temperature Min: **20.4 °C**
 Temperature Max: **21.4 °C**

Strict Acceptance:
 1 Point: **0.0046+0.0020L/1000**
 2 Point: **0.0047+0.0019L/1000**

Strict Acceptance Limit from E0 and E150 Results

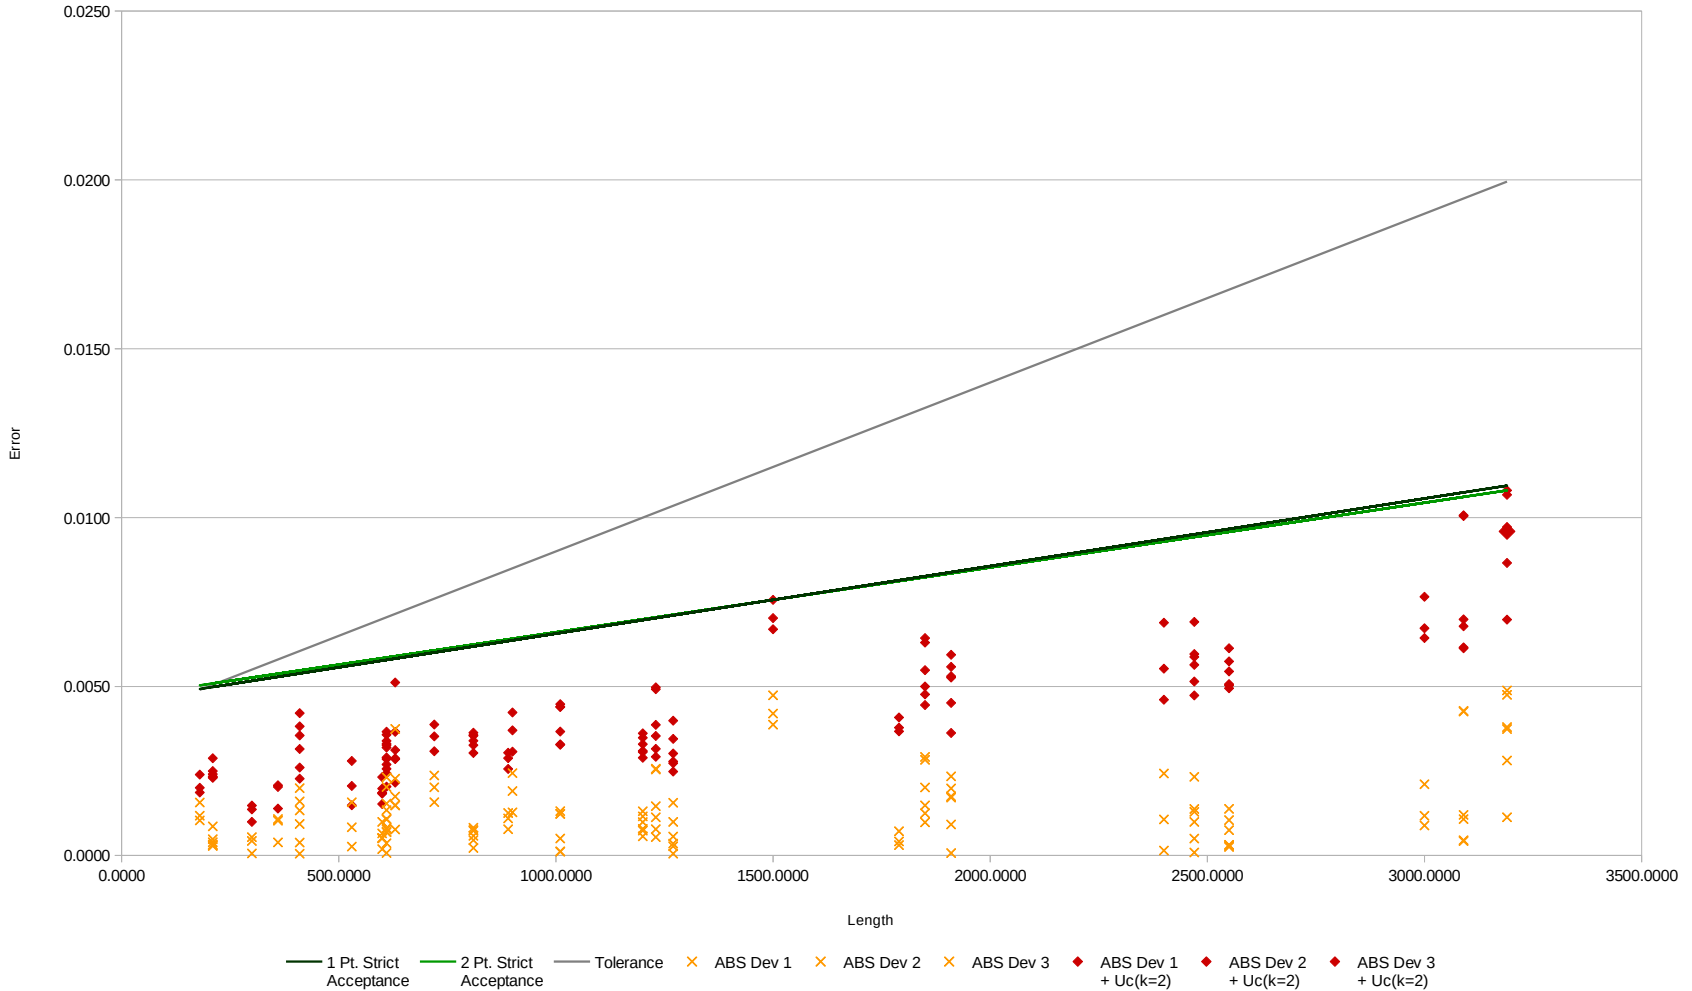

Calibration Workspace 9.0